(54) Title: FUNCTIONAL ELECTRICAL THERAPY SYSTEM (FETS)

(57) Abstract: The Functional Electrical Therapy System (FETS) relates to an apparatus and the method of its application for recovery of upper limb functioning in humans with sensory-motor lesion in the central nervous system having impact to reaching and grasping. The recovery is contributed by 1) the electrical stimulation of efferent nerves that augment and/or generate missing functions of the upper limb, 2) electrically induced strong input to the central nervous system via afferent nerves, 3) intensive exercise by the same paretic upper limb, and 4) increased awareness of being able to accomplish the task. The methods comprise the use of the novel apparatus that provides missing or diminished functions of the upper limb during intensive daily exercise of performing typical daily activities that requires these functions. The FETS consists of a multi-channel stimulator, set of surface electrodes, and the novel controller that mimics spatial and timing synergies of muscle activation found in able-bodied subjects when performing functional tasks.

FUNCTIONAL ELECTRICAL THERAPY SYSTEM (FETS)

5   The present invention relates to a method and to apparatus for improving the physical ability of persons having disabled upper extremities due to sensory-motor impairment of the central nervous system.

The motor functions of an upper limb that is paretic or 10 paralysed after stroke can be improved by intensive exercise and augmented feedback [Sunderland et al., 1992], or Constraint Induced Movement Therapy [Kunkel et al., 1999; Miltner et al., 1999, Taub et al., 1999]. The use of robots can also enhance the motor functioning [Aisen et al., 1997; 15 Volpe et al., 2000]. Electrical stimulation of peripheral sensory-motor systems works as a therapy, although there are no conclusive directions which technique works the best for a given indication [Kraft et al., 1992; Glanz et al., 1996; Hummelsheim et al., 1997; Feys et al., 1998; Chae et al., 20 1998; Francisco et al., 1998; Dimitrijevic and Soroker, 1994; Dimitrijevic et al., 1996; Sonde et al., 1998, 2000]. Electrotherapy was introduced by Liberson et al. [1961]; they used a peroneal stimulator to provide contraction of the dorsiflexor muscles based on the trigger signal that 25 came from the heel switch in order to reduce the foot-drop.

In an early use of electrotherapy in upper limbs Merletti et al. [1975] applied a two or three channel electrical stimulator to augment elbow extension and fingers/wrist extension. The device used proportional 30 control, and it allowed independent control of each of the stimulation channels. The patients were hemiplegic. With stimulation, they were able to move an object from one

location to another, which they could not do without the
stimulation. The conclusions from this small clinical trial
were that an improvement was obtained in elbow extension
without stimulation over a period of three months, but not
5 of hand opening movement. The conclusions from a small
clinical trial were that the electrotherapy improved the
hand and elbow control with stimulation in all study
subjects.

Stimulation systems for functional support of the upper
10 extremities have been developed for spinal cord injury and
stroke, both implanted and with electrodes attached to the
skin. In many cases, these systems have been developed to
provide immediate functional support, although beneficial
therapeutic effects, resulting in improved voluntary
15 movement control, have been reported in several studies.
More recently, studies have been performed that investigate
the therapeutic effect of electrical stimulation primarily.
The neurophysiological basis of these therapeutic effects is
still insufficiently understood. Therefore, it is unclear
20 how the therapy should be optimized.

There are several stimulation systems that use several
surface electrodes, multi-channel stimulator and a pre-
programmed sequence of stimulation that can be triggered by
a switch, several switches, or signals from a sensor
25 [Nathan, 1993, Ilic et al., 1994; US 5330516; Saxena et al.,
1995; Prochazka et al., 1997; US 5562707; Popovic and
Popovic, 1998; Popovic and Popovic, 2001; Fisekovic and
Popovic, 2001]. There are several stimulation systems with
implantable electrodes [Hoshimiya et al., 1989; Smith et
30 al., 1987], or fully implantable systems [Smith et al.,
1996; US-A-5167229] that use a pre-programmed stimulation
that is controlled by a switch or sensory signal in an open-

loop or closed-loop control scheme. These stimulators have
been designed to operate in humans with chronic paralysis or
paresis caused by a cerebro-vascular accident or spinal cord
injury (e.g., Popovic et al., 1998; Popovic et al., 1999].
5 All of these stimulators use the well-known principles
described basically in the work of Liberson et al., [1961]
and Rebersek and Vodovnik [1973]. Most of the stimulation
systems comprise the flexibility to be programmed for
various applications other than the one that they are
10 originally designed for; however, the best stimulation
protocol is unknown thus the change of the stimulation
protocol is not straight forward.

In a first aspect, the present invention provides a
method for integrating electrical stimulation and upper
15 extremity exercise in order to improve the physical ability
of persons having a disabled upper extremity due to sensory-
motor impairment of the central nervous system, said method
comprising the steps:

- imposing from the apparatus functional electrical
20 stimulation of neural pathways based on a voluntary command
using a stimulation pattern that mimics natural flow of
neural activities to the impaired upper extremity,

- generating the missing components of a functional
movement in parallel with the voluntary exercising of the
25 same functional movement based on the said patterned
stimulation of the efferent neural pathways time-
synchronized with volitional movement,

- enhancing the afferent input by the said patterned
electrical stimulation in time synchrony with the biological
30 afferent activity caused by the functional movement of the
limb.

Most of the previously described techniques considered
only to a peripheral degree the manner in which the
different treatments benefit from the today very well
accepted effects of neural plasticity. Namely, the human
5   brain has a power to change its structure and function in
order to optimize the performance of frequently performed
activities. The brain learns from its own actions. The
afferent sensory information, giving feedback about the
consequences of voluntarily controlled actions, is essential
10 for this learning process. It is the way young children
learn to move in a functional manner, or professional train
for competition. There is increasing evidence that it is
also the way adult persons relearn their motor activities
after a stroke.

15   Therapy for motor relearning in persons with paresis
caused by stroke should support this process of relearning
optimally by functionally assisting the user to perform
intended activities, which they may only be able to perform
poorly or not without assistance. The sensory feedback
20 associated with the performance of the activities will
assist the relearning process of the brain. This functional
sensory feedback should be maximized both in intensity and
duration and should not be limited to short clinical
training sessions.

25   Functional Electrical Therapy (FET) in accordance with
this invention is the ideal modality for this activity
dependent neurorehabilitation. FET is (in preferred aspects)
a non-invasive neuromuscular stimulation modality that
assists motor activities intended by the user, while
30 activating sensory channels that provide maximal afferent
inflow to the brain, consistent with the performance of the
activities, thus training the neuromuscular system to

perform the function independently. FET trains function in
contrast to conventional electrical therapy. The FET
approach promotes functional reorganization of the brain
and, consequently, functional relearning. During the therapy
5   period, a FET system can be provided to each stroke person
for use during his or her daily activities, thus resulting
in intensive training. Recent studies suggest that FET is a
promising modality for promoting the relearning of reaching
and grasping in paretic persons [Popovic et al., 2002].

10   Functional Electrical Therapy (FET) enables a paretic
user to perform functional activities during a period when
he-she is not yet able to perform these functions self-
sustained, thus promoting normal functioning. The functional
sensory information thus generated is hypothesized to result
15 in intensive functional brain training of the activities
performed. The functional support and maximal sensory
functional feedback to the spinal cord and the brain make
FET very different and, preliminary data indicate, superior
to alternative forms of traditional therapies (neuromuscular
20 facilitation, therapeutic neuromuscular stimulation, below
the motor threshold stimulation, intensive exercise, etc.).

    Although general theories exist regarding the
neurophysiological basis of neurorehabilitation through
Functional Electrical Therapy, limited actual knowledge is
25 available about the mechanisms.

    Conceptually, the following processes are believed to
contribute to the training of the neural and muscular
systems when applying Functional Electrical Therapy:

•   Arm muscles are activated in a functional manner through
30   the stimulation of the peripheral motor nerves. In this
        way, functional activities, which may not be feasible
        without support, can be performed. Furthermore, the

stimulation results in strengthening of the activated
paretic muscles.

- The body's sensory system generates sensory signals
  providing information about the performance of functional
5 activities.

- Sensory signals are furthermore generated directly by the
  excitation of sensory nerve fibers in the stimulated
  peripheral motor nerves.

- The sensory information generated by the body's sensory
10 system and through direct nerve stimulation influences the
  neural networks in the spinal cord, with impact on the
  reflexive system, possibly reducing hyper-reflexia and
  functionally modulating reflexive pathways.

This sensory information furthermore influences the
15 structure and function at the level of the brain,
potentially improving volitional motor control performance
by learning.

Thus, in accordance with the method of the invention,
patients having a deficit in the brain, typically of the
20 type induced by a stroke, rather than in the efferent nerves
of the spinal cord or lower, benefit from FETS. By a
'functional movement', we mean a desired, previously
determined movement, such as opening the hand, engaging an
object and closing the hand to grip the object.

25   In accordance with the method, the patient wills the
functional movement to occur and attempts to make the
movement by voluntary action of the relevant muscles for
performing the movement in the healthy person, at the same
time that the apparatus produces the movement by a pre-
30 programmed electrical stimulation of the muscles. Thus, the
patterned stimulation of the muscles is synchronised with
volitional movement or volition of movement (whether or not

the patient is capable of any relevant movement without the
stimulation).

The electrical signals are perceived by the patient,
which provides an enhanced afferent input in synchrony with
5 biological afferent activity, i.e. exteroceptive signals as
well as proprioceptive signals.

The Functional Electrical Therapy System (FETS)
comprises an apparatus and the method of its application for
recovery of sensory-motor systems in humans central nervous
10 system injury with impact to reaching and grasping that
combine the both techniques: electrical stimulation and
exercise. An important preferred feature of the FETS is the
control that allows that the electrically elicited activity
of hand and arm of a person with sensory-motor deficit is
15 synchronised with the extensive exercise; thereby affecting
all available resources and leading to the fast and
efficient rehabilitation of function [Popovic et al., 2001].
The FETS is designed for short-term therapeutic application;
it is not developed for chronic, every day orthotic use
20 alike Freehand[©] [Smith et al., 1998] or Handmaster NMS-1[©]
systems [Nathan, 1993].

In a preferred method according to the invention the
electrical stimulation is provided from the stimulator at a
number of the bodily locations by means of surface
25 electrodes. However, the use of implanted electrodes is not
excluded.

Preferably, the efferent pathways are pathways from the
spinal cord of the disabled person to a muscle in the arm or
hand of the disabled person.

30 A control algorithm is preferably incorporated into the
controller, said control algorithm mimicking the natural
sequence of activation of muscles responsible for functional

movements. The mimicking may provide stimulation comprising
triphasic activity of agonist muscles and antagonist muscles
and controlling the level of co-contraction of agonists and
antagonists.

5   A voluntary movement in the same upper limb may be used
as a source to drive in an open-loop control scheme the
activation of more distal parts of the arm. Such movement
may be the moving forward of the elbow in a reaching
movement.

10   The afferent pathways may be pathways from the sensory
system of the body of the disabled person to the spinal cord
of the person.

         The steps may be repeated so that the electrical
stimulation for a prolonged time provides a strong afferent
15 input that is correlated with the propriceptive and
exteroceptive inputs caused by the voluntary movement and by
contacts with the environment.

         The invention provides in a second aspect apparatus for
use in the integrated electrical stimulation and upper
20 extremity exercise in order to improve the physical ability
of the upper limb of a disabled person, said apparatus
comprising a stimulator for providing electrical signal
outputs via a number of stimulation channels, and a number
of electrodes for placement in physical contact with the
25 body of the disabled person and means for connecting said
electrodes to said stimulator, and a controller providing
instructions to said stimulator and implementing a control
algorithm that causes the stimulator to provide via said
channels stimulation patterns of said electrical signals
30 which induce muscle movements in use which mimic the timing
and modulation of muscles typically active in able-bodied
humans that are available for surface activation with

electrical stimulation in persons with impairment, said
signals including non-simultaneous peaks of activation of
agonist and antagonist muscles during a single direction of
movement (triphasic pattern) and appropriate coactivation of
5 agonist and antagonist muscles needed for a desired
functional movement.

Said apparatus may be suitable for use in performing
the method of the first aspect of the invention. Suitably,
the apparatus is suitable for producing manipulation and
10 grasping of objects with an impaired hand.

The controller may communicate with a number of
stimulators, said stimulators comprising lead communication,
alternatively or supplementary wireless communication
channels between the controller and stimulation points.

15 The apparatus may be intended for stimulating and
controlling fingers, thumb, and forearm of the disabled
person, and the number of stimulator channels may comprise
at least one channel for the finger flexors, at least one
channel for the finger extensors, at least one channel for
20 thumb extension/adduction, and at least one channel for
thumb opposition/flexion.

The apparatus may comprise a shoulder angle sensor for
determining the angle or rate of change of the angle between
the upper arm and a reference line, wherein said controller
25 is adapted to initiate and to regulate a said control
algorithm inducing a sequence of reaching, grasping, moving,
holding, returning and releasing an object in response to
measurement or calculation of said rate of change based upon
the output of said shoulder sensor.

30 The invention further includes the use of the apparatus
for improving the physical ability of persons having
disabled limbs due to sensory-motor impairment in the brain

of the person caused by a lesion of the central nervous
system of the person, where the improvement relates to long-
term changes of ability to perform movement without the
stimulation after the treatment.

5   Also, the invention includes the use of apparatus for
temporary therapeutic applications in persons with sensory
motor deficit of an upper limb within the intensive physical
exercise, said therapeutic application augmenting and/or
generating the missing movement of the hand/arm.

10   The invention will be further described and illustrated
with reference to the accompanying drawings in which:

        Figure 1 shows the organisation of a rule based
synergistic control for a preferred embodiment of the
invention at coordination and actuation levels for FETS;

15   Figure 2 shows a schematic of the central
stimulator/controller of the described preferred embodiment;

        Figure 3 shows a stimulation map indicating the timing
of electrical stimulation to muscles involved in a drinking
movement; and

20   Figure 4 shows a similar stimulation map for a modified
embodiment providing fewer channels for electrode
stimulation and provision for input from a shoulder angle
reading sensor.

        A Functional Electrical Therapy Apparatus comprises the
25 following 1) a multi-channel stimulator that is capable of
activating paralyzed innervated muscles when applied with
surface electrodes, 2) a controller that is capable of
generating command signals that would fit into the
biological control of movement. 3) electrodes, 4) sensors,
30 and 5) switches.

        1) A multi-channel stimulator that allows stimulation
of motor nerves can be used for that providing that it can

be controlled in sense of frequency of stimulation, pulse
duration, and pulse amplitudes.

The therapeutic stimulation uses pulses that are about
200 microseconds long, have amplitude in the range of 0 to
5 50 mA, and the frequency of 50 Hz. These parameters have
been selected in order to minimize the pain, yet decrease
the development of fatigue. The therapeutic stimulation is
not meant for static applications (e.g., long lasting
grasps), yet for the dynamic behaviors (e.g., move, grasp,
10 release during functional use of objects typically needed in
daily life).

Communication link to the controller allows that this
stimulator generates specific bursts of activities that
could generate various movements. This link allows control
15 of pulse duration and stimulation frequency on each of the
channels independently. This means that each channel can be
turned at any time at any intensity depending on the control
signals delivered through the said link.

2) FETS controller uses a coordination model of
20 movement that has been described in literature dealing with
motor control [Popovic, 2002].

The coordination model of reaching and manipulation
hypothesizes that there is a high connectivity between
individual joint movement that is, muscle activation during
25 functional movements. The connectivity is being developed
through a skill acquisition procedure, mostly in childhood.
This connectivity allows that a single decision at the brain
level to perform a function is appropriately distributed to
end organs. This coordination is achieved by the
30 hierarchical and parallel organization of the CNS, yet is
can be assessed and presented in different phase spaces
(e.g., force space, velocity space extrinsic or intrinsic

coordinates). Control of reaching and grasping was found
independent (reaching and grasping synergies) [Jeannerod,
1981], but coordinated through a hierarchically higher
control mechanism that ensures temporal alignment of

5   reaching and grasping. Dissociation in the control of
reaching and grasping was confirmed in comprehensive studies
[Gentilucci et al, 1997]. Neurophysiological findings
support functional separation of reaching and grasping [Van
Kan et al, 1994]. Decoupling between the reaching and

10 grasping controls is suitable for life-like control yet
temporal synchrony between the reaching/grasping/releasing
movements stays instrumental.

        Conventional control techniques developed for machine
and robots are not suitable for the multi-joint, multi-

15 actuator biological systems such as the arm/hand complex
[Tomovic et al., 1995; Potkonjak et al, 2001] mostly because
external control must be integrated into the preserved
sensory-motor mechanisms. Incorporating preserved natural
features and generating artificial life-like control

20 requires the use of heuristic tools and structuring control
in a hybrid hierarchical fashion [Tomovic et al, 1995].

        A coordination model of control is shown in Fig. 1; it
comprises three automatic, and one biological control level
[Popovic, 2002]. The highest control levels (decision and

25 planning) allow the user of a neuroprosthesis to select an
action, and the modality of operation, i.e. to provide
sufficient detail to specify where, how, and what the
movement should accomplish. The role of the second automatic
level is to coordinate simple synergies between joints and

30 it could use a discrete rule-base control. A rule-base
controller operates as a sampled-data feedback system, and
its role is to transfer commands to the lower level and

process the feedback information. A rule-base controller implements the state model of movement that is cloned by a heuristic of machine classification using data acquired in able-bodied humans; thereby mimicking life-like movement.

5   The rules need to be determined with sufficient generality to allow the application over a large population with minimum limitations. The lower coordination is implementing synergies at the joint level, *i.e.*, machine determined mappings between the state variables (e.g., arm
10 segment angular velocities) [Popovic and Popovic, 1994, 2001]. The lowest, actuator level deals with execution, that is, for example, patterns of functional electrical stimulation of muscle groups being responsible for the flexion or the extension of a single joint, or biarticular
15 muscles contributing to the movements of the neighboring joints. The actuator level implements open-loop model-based control than includes individual biomechanical and neuromuscular features of the eventual user.

The FETS deals with two motor system properties of
20 manipulation and grasp: 1) Temporal synchrony; and 2) Reaching synergies.

1. *Temporal synchrony*. The execution of manipulation and grasp functional task is coordinated through the following phases: 1) the hand transport to the object post
25   (positioning or reaching), hand orientation and opening (prehension), hand closing (grasping of the object); 2) using the object (the actual task); 3) returning the object and releasing it at the object post; and 4) finally returning the hand to the initial position.

30 2. *Spatial synergies*. The term spatial synergy means acting together. This can be linked to low-level neural elements (reflex arc), only one step away from the muscle

[Sherrington, 1947] or alternatively, at higher-level neural processes *i.e.* functional [Bernstein, 1967]. The synergy can be anticipated at the level of movement initiations, that is activation of muscles, or at the

5   level of movement performance (execution), that is individual joint rotations [Latash *et al*, 1999]. Spatial synergy is a rule that establishes a relation among central control variables to individual joints of a limb resulting to a relation among performance variables.

10 Existence of synergies is expected to shift control of multi-joint movements to a higher level, as compared to control of individual joints, and to decrease the number of central variables manipulated by CNS.

There is no other therapeutic system that uses this

15 mode of control. Control algorithm provides alternating stimulation of agonist and antagonist muscles in the order typically found in able-bodied subjects. Control algorithm comprises phases of cocontraction and typical triphasic activity of muscles.

20   Thus, it can be seen in Figures 3 and 4 that during a phase of the desired complex movement in which the movement of a component of the limb, such as the fingers, is in a single direction, e.g. opening of the fingers, the stimulation of the muscles involves peaks of stimulation of

25 agonist and antagonist muscles which follow one another. This is further described below.

The tested controller (Fig. 2) is powerful; it is capable of regulating up to 8 bipolar, mutually independent stimulation channels. The outputs from the controller are

30 logical signals: Low and High. The interpulse interval, reciprocal of the frequency of stimulation, is the time between two subsequent transitions from Low to High; it can

be selected to be between 10 ms and 2,55 seconds in increments of 10ms. The pulse duration is equal to the period of a single "High" state; it can be programmed to be between 10 s and 1270 s in increments of 10 s. The

5 increase and decrease rates of pulse duration are programmable for each of the channels independently. The amount of charge delivered to the motoneurons depends directly on the pulse amplitude, which is set at the stimulator output stage manually. The power generator and

10 output stages anticipated for FES system are a modified version of the stimulator developed by Ilic *et al*. [1994].

The controller operates in a sensory-driven mode, data from analog sensors are fed to an 8-bit A/D converter (a component of the micro-controller), and/or digital signals

15 from digital sensors go directly to a port on the micro-controller. The controller supports up to a maximum of 6 digital and 8 analog sensors. The sensory output signals must be processed to be between 0V (Low) and 5V (High). Five fully retriggerable timers are integrated in the controller

20 in order to enable the use of a time series of sensory data and special commands. The timers are designed for the range between 0.05 to 50 seconds, with an increment of 0.05 seconds. In order to increase the control capacity, five internal control signals can be generated and stored in the

25 memory of the micro-controller. These control signals define the state of the stimulator and allow multi-modal operation (*i.e.* different patterns can be activated for the same sensory input). The timers and control signal are important specifically for the application of a hierarchical hybrid

30 rule-based control [Popovic and Sinkjær, 2000].

The controller comprises the following: a micro-controller, two programmable logic arrays, a flash memory,

an infrared (IR) communication port, and a time base

generator. The PIC16F877-20I/PT micro-controller is the core

of the device (Fig. 2). It co-ordinates all other sections

and executes the algorithms. The controller digitises input

5 signals from analog sensors and/or receives digital signals,

generates part of the address for access to the flash

memory, and forwards the appropriate data to the

programmable logic arrays.

Two programmable gate arrays (PGA) perform logic

10 operations. The basic tasks for PGA chips are to generate

pulses with defined duration on the basis of information

received from the micro-controller. The PGA chips also deal

with the logic for the bus control, access to the

peripherals and memory modules, and they serve as the

15 interface for the digital sensors.

Intel's flash memory DA28F016SV (capacity 2 MB) was

selected based on the estimated size of the programs. The

flash memory was preferred to a ROM memory because of the

needs to tune and change the programs on site. The process

20 of reading flash memory is the same as reading SRAM with

respect speed and access, yet the content remains in the

memory after the system is switched off.

The controller and PC communicate via an IR transceiver

[Fisekovic and Popovic, 2001]. This cordless communication

25 is only for transmission of the control algorithm (generated

at a PC computer) to the stimulator. The IR communication

system comprises an infrared transceiver (MINI SIR,

Novalog), and the pulse shaping circuit (IC transceiver

driver, TOIM3232, Temic). At the PC side there is a MAX232

30 (Maxim) level conversion chip between the serial port (RS232

standard: ±12V), and the transceiver drivers (5V). The IR

transceiver MINI SIR and the circuit TOIM3232 are compatible
with IrDA association standards.

In order to simplify the pulse generation a timer
(LMC555) is configured for operation as a system basic
5 rhythm clock (self-oscillating flip-flop) at the frequency
of 100 kHz, ensuring the minimum pulse duration of 10 μs.

The operation principle of the controller is the
following: the data from analog sensors are fed to the
microcontroller inputs, and transformed to a digital form.
10 Based on these values, the timer states, and the control
register states, the microcontroller generates part of the
address for access to the flash memory. This part of the
address consists of 16 lower bits, out of a total of 22 bits
needed for the access to the memory (21 address bits, and 1
15 bit for chip selection). The structure of this part of the
address is as follows: the six lowest bits define the data
from the control algorithm that is currently read, and the
channel to which the reading applies. The nine following
bits are distributed among A/D converters, timers, and
20 control signals, and the distribution is defined by the
stimulator configuration. These nine bits are actually
defined by the current state of input and control values of
the stimulator, and they determine the action that should be
performed by the control algorithm. The sixteenth bit
25 represents chip selection, and it defines whether the next
instruction from the micro-controller program is read in the
current memory cycle, or whether the flash memory is
accessed and data defined by the control algorithm are read.
The program generates the remaining six address bits on the
30 basis of the states of digital sensors. A combination of
these six bits and the nine bits generated by the micro-
controller defines the immediate control data. These data

are sent to the programmable logic arrays (frequency and
pulse duration). Then, the new timer states and control
signals are set. Finally, the pulses generated by the micro-
controller are fed to opto-couplers that drive the output
5 stages of the stimulator. Based on the data read, the micro-
controller also selects the channels that should be active.

The interface program for entering the control
algorithm and its parameters is supported by Windows
operating systems with the minimal hardware requirements (PC
10 based computer with a VGA graphics card).

The programmer initialises the set-up, and he/she is
prompted with the main menu. The menu enables selecting one
of the following six program activities: 1) configuration,
2) algorithm definition, 3) program file, 4) generation of
15 the stimulator code, 5) load and save, and 6) exit, as
follows:

1) Configuration. This section of the program is used
to define the actual configuration of the stimulator for the
selected operation: active A/D channels and their range,
20 timers and control signals that will be used, number of
channels that will be used, and unipolar or bipolar regimes.
It is desirable to decrease the large number of input signal
levels with a smaller set of values [Tomovic et al., 1995];
thus, 2, 4 or 8 levels of analog signals are allowed. In
25 order to minimise effects from the noise recorded by sensors
and noise introduced by the A/D conversions, a hysteresis of
the sensory signal readings was introduced: an upper and
lower threshold defines each sensory level. The
configuration section of the program is used to choose how
30 many levels will be used. The software automatically checks
for contradictory configurations.

2) Algorithm definition. This section is the main part
of the program. It allows the user to define the conditions
and appropriate modality of stimulation. The combination
defined by the states of the sensors (digital and analog),
5 timer, and control signal states is entered in the
definition of the algorithm. The definition of the algorithm
opens a mask where the programmer sets the pattern of
stimulation. This section allows setting of the minimum,
maximum, rise, and fall times of pulses for each channel
10 independently, and it allows the set-up of the interpulse
intervals. This programming applies when the stimulator is
to be used for therapy and exercise. The algorithm
definition is automatically downloaded from the machine
learning program for functional movements like walking
15 [Jonic *et al.*, 1999].

3) Program file. This section offers two possibilities.
The first is named *condition check.* By starting this option,
the program examines whether there are contradictions in the
control algorithm (e.g., more than one pattern of
20 stimulation is defined for the same set of input
parameters). If contradictory conditions are detected, the
program informs the user about the conditions that are
contradictory, and they have to be manually corrected. The
second option is *program file generating.* This option
25 generates a file containing data formatted to suit the
micro-controller.

4) Stimulator programming. This section is used for
transferring the file from the PC computer to the micro-
controller memory.

30   *5) Load and save.* This section allows the programmer to
save the defined program on the PC computer for later use.

It is possible to save the control algorithm and the stimulator configuration, or only the configuration.

6) Exit. This section closes the programming sequence and prompts the programmer to the unsaved information before 5 exiting.

The control algorithm provides a so-called life-like control. The operation of the controller can be classified to sensory-driven or switch-triggered open-loop procedure [Popovic and Popovic, 2001, Tomovic et al., 1995]. The 10 control delivers signals that sequentially activate programmed bursts of electrical pulses to agonist and antagonist muscles of distal arm segments. The cathodes are positioned so to deliver charge to finger flexors, finger extensors, thumb extensor and flexors following the grasping 15 synergy and the timing that mimics the movement seen in healthy subjects when reaching and grasping. The key element is the timed activation of finger and thumb extensors for palmar and lateral grasps that provide opening during the prehension phase, and time activation of thumb and finger 20 flexors during the closing phase of the grasp. The control algorithm incorporates the control of pronation and supination of the forearm, as well as elbow flexion/extension, yet they do not have to be employed if so decided.

25   The actual change of the pattern (grey areas) is obtained by the change of the pulse duration in real-time. The stronger the stimulation needs to be the longer the pulse should be. The adjusting of the pulse duration vs. the generate movement is individual. The controller of the FETS 30 uses a template type adjusting; patients tune is by adjusting the overall intensity of the pulse intensity, that

is, they are setting the level to which all signals are than normalised.

The actual change of the pattern (grey areas) is obtained by the change of the pulse duration in real-time.
5 The stronger the stimulation needs to be the longer the pulse should be. The adjusting of the pulse duration vs. the generate movement is individual. The controller that is part of the FETS uses a template type adjusting, it is not tuned to each patient wit the pulse duration; patients tune is by
10 adjusting the overall intensity of the pulse

The graph presented shows two important elements. There is two couplings: 1) a coupling between the intensity of stimulation and movement in proximal joint at the level of control of reaching (elbow movement, pronation/supination),
15 and 2) timing coupling between the onset of stimulation for opening and closing of the hand coming for the sensor on the proximal muscle, or from a switch if the proximal segments are not instrumented with electrodes or sensors.

The controller is responsible for, as shown in Figs. 3
20 and 4, alternating and/or simultaneous, if so required, stimulation of agonist and antagonist muscles.

The control scheme was developed based on detailed analysis of able-bodied persons movement during functional tasks. The subjects were seated in front of a desk and asked
25 to slowly do many manipulation and grasping tasks. The tasks (e.g. drinking from a full juice can and small bottle, handling a video-cassette and CD, writing with a pen, eating finger food) were selected to include the following: 1) palmar, lateral, and precision grasp; 2) different positions
30 within the working space defined with the following attributes: distance and laterality, and 3) various sizes and weights of objects.

The volunteer subjects were asked to repeat for five times each functional task using their dominant arm. Four subjects were left handed, and six right handed. The data was recorded in all subjects during three independent

5 sessions. The order of tasks was randomly changed. Subjects were asked to slowly move their arm while performing a task (drink, eat, write, etc). Subjects were instructed to stop their movement once they accomplish the grasp, at the moment that they start the functional use of the object (e.g.,

10 drink, write), and at the time after they released the object at the object post.

Data were collected (three dimensional movement analysis) and off-line processed. The processing provided the tabulated angular velocities that could be automatically

15 analyzed. The task of analysis was to determine the minimal number of unique coupling between joint angular velocities that characterize the task, position, size, or their combination. Two forms of couplings were of interest: the spatial mapping and the time synchrony. The duration of

20 movement duration was normalized for each series of measurements. We used advanced machine learning techniques for determining the couplings between the joint angular velocities, as well as the timings between different events to be controlled.

25 The second element for designing control was to analyze the stimulation pattern that is required to produce different movement when using surface stimulation. The method for designing stimulation patterns was described in details in Popovic et al. [1994]. The method assumes a

30 series of measurements in the potential user for determining joint and muscle properties. A detailed analysis of joint and muscular properties in many stroke subjects showed that

it is possible to define the stimulation pattern with respect the maximum stimulation level, and that it is sufficient to divide the subjects in the group of highly spastic, moderately spastic, and minimally spastic strokes.

5   This allowed the simplified design of FETS control that requires only individual adjustment of the maximum stimulation level (hand controlled potentiometer on the FETS), while the remaining adjustments are done automatically.

10   3) Set of electrodes being safe for delivering electrical charge for periods of approximately 30 minutes two times a day for a limited interval (e.g. 6 weeks).

These electrodes are daily positioned by the therapist or other trained professional. The electrode system does not
15 require self-mounting. The reusable polymer based electrodes are likely to be the best choice. The size of an electrode has to be individually selected and sized based on the required position on the hand, forearm, or upper arm, the size of the hand and arm, and degree of atrophy. This system
20 is meant for stroke patients; thus, they are capable of positioning of the electrodes on their own with the good hand once they are trained where to place the electrodes.

The simplest system requires the use of four stimulation channels applied via 5 or 6 electrodes. The
25 cathode for the extension of fingers (opening of the hand) is positioned over the muscle nerve of extensor digitorum communis, and the anode over the bulk of the muscle. The cathode for fingers flexion is positioned over the muscle nerves for flexor digitorum profundus and superficialis,
30 while the anode is positioned over the ulnar and median nerves. The channel responsible for the extension of the thumb is positioned over the muscle nerve of the extensor

pollicis longus and the anode over the ulnar and median nerve. Finally the channel that provides thumb closure is positioned over the thenar muscle group.

The more complex system includes four more channels for
5 stimulation that control pronation/supination (cathodes are positioned over the pronator and supinator muscle nerves, and the anodes over the bulk of the muscles. The remaining two channels control the elbow flexion and extension. The electrodes are positioned over the biceps brachii and
10 triceps brachii muscles. The exact positioning must be determined on the individual basis by using specially designed probe that is used as a cathode. The positioning once determined changes very little, yet the individual differences are substantial preventing in having a universal
15 electrode holder or similar interface.

4) Sensors for the system detect the joint angle. The sensors used in this system are goniometers that supply data used to determine the elbow and shoulder flexion/extension angular velocities. The goniometer is not part of this
20 invention, yet its used is.

The role of the sensor is shown in the Fig. 3. The figure shows the operation of eight channels for functional drinking.

The top panel shows the angular velocities measured at
25 the shoulder joint. The angular velocities can be measured directly or estimated in real-time from the joint angle measurements. The joint angular velocities are used for two purposes. When the joint angular velocity crosses the threshold for both positive and negative joint angular
30 velocities (shaded rectangle at the top panel, Fig. 3), then the timing is determined that triggers the required activity (e.g., first flexion starts the prehension and approach

phases in all shown muscles, and when this flexion angular velocity becomes small enough the reach phase is over). The joint angular velocity is in parallel used with the predetermined mapping to control in feed-forward manner the

5 pronation/supination and elbow flexion/extension. The first extension that is bigger than the threshold starts the "move" to the functional use phase. The second flexion crossing starts the forearm orientation for accomplishing function. The third flexion angular velocity crossing of the

10 threshold starts the return phase of the hand in order to release the object used. A very short over the threshold extension triggers the mid release phase. Finally the last extension crossing of the threshold starts the relaxation phase.

15   The functional drinking includes reaching to the object with adequate orientation of the hand, opening of the hand, adjusting the hand for a firm grasp, bringing the object to mouth, rotating the object in order to drink, drinking the object to the object task, releasing the

20 object, returning of the hand to the initial position, and relax state. One can extract any combination of the channels to be used based on the specific needs of the given patient. The reduced number of channels uses the same schema, yet less than eight channels are connected to electrodes.

25   5) A switch may be provided for initiating operation of FETS. The switch provides the instrumental interface to the user. The switch turns on and off the operation and allows intervention at any time. Such a switch is at a higher level of control than sensors. Any switch that provides instant

30 operation and has the de-bouncing properties can be used within the system.

An example of using only the four channels that control the grasp is presented in Figure 4 and it is a subset of the channels shown in Figure 3.

Figure 4 shows the timing when switch triggers the
5 activity (arrows). A sequence of grasping is divided to the prehension phase (opening of the hand and shaping it correctly for the object size and shape), and grasp where firm contact and safe grasp are accomplished. The grasp phase will last as long as the subject does not trigger the
10 release phase. The pattern of stimulation is not straightforward; it was designed to follow the triphasic pattern of activity that promotes the smooth movement, yet also the enhanced activity of afferent pathways. In parallel, the necessary levels of cocontraction provide
15 smooth and safe graph in addition to ability to fast respond to possible need for changing the posture of the hand.

Thus, it can be seen that upon operation of the switch a sequence of stimulating pulses is sent to each electrode. Looking first at the pulses sent to the finger flexion
20 producing muscles (upper panel, dark grey) it can be seen that the intensity of the pulses (represented by the height of the shaded area above the baseline at any instant) increases rapidly to a peak. Simultaneously with this, pulses sent to the antagonist muscles controlling extension
25 of the fingers (upper panel, light grey area) increase slowly to a peak spaced in time from the agonist stimulation peak. Then the stimulation of the antagonist muscles is sharply reduced, whilst the stimulation of the agonist muscles rises again to a subsequent peak. This alternation
30 of peaks in the stimulation of the agonist and antagonist muscles can be seen to characterise all of the phases of movement.

Thus in summary, a preferred aspect of the invention is the provision of a Functional Electrical Therapy System (FETS) which relates to an apparatus and the method of its application for recovery of upper limb functioning in humans
5 with sensory-motor lesion in the central nervous system having impact to reaching and grasping. The recovery is contributed by 1) the electrical stimulation of efferent nerves that augment and/or generate missing functions of the upper limb, 2) electrically induced strong input to the
10 central nervous system via afferent nerves, 3) intensive exercise by the same paretic upper limb, and 4) increased awareness of being able to accomplish the task. The methods comprise the use of the novel apparatus that provides missing or diminished functions of the upper limb during
15 intensive daily exercise of performing typical daily activities that requires these functions. The FETS consists of a multi-channel stimulator, set of surface electrodes, and the novel controller that mimics spatial and timing synergies of muscle activation found in able-bodied subjects
20 when performing functional tasks.

References

1. Aisen ML, Krebs HI, Hogan N, McDowell F, Volpe BT. The
   effect of robot-assisted therapy and rehabilitative
   training on motor recovery following stroke. *Arch Neurol*
   54:4 443-6, 1997.

2. Bernstein NA. *The coordination and regulation of
   movements*. London: Pergamon Press, 1967.

3. Chae J, Bethoux F, Bohine T, Dobos L, Davis T, Friedl A.
   Neuromuscular stimulation for upper extremity motor and
   functional recovery in acute hemiplegia. *Stroke* 29:5 975-
   9, 1998.

4. Dimitrijevic MM, Soroker N. Mesh-glove 2: Modulation of
   residual upper limb motor control after stroke with whole-
   hand electric stimulation. *Scand J Rehabil Med* 26:4 187-
   90, 1994.

5. Dimitrijevic MM, Stokic DS, Wawro AW, Wun CC. Modification
   of motor control of wrist extension by mesh-glove
   electrical afferent stimulation in stroke patients. *Arch
   Phys Med Rehabil* 77:3 252-8, 1996.

6. Feys HM, De Weerdt WJ, Selz BE, Cox Steck GA, Spichiger R,
   Vereeck LE, *et al*. Functional magnetic resonance imaging
   of the human motor cortex before and after whole-hand
   afferent electrical stimulation. *Scand J Rehabil Med* 31:3
   165-73, 1999.

7. Fisekovic N, Popovic DB. New Controller for Functional
   Electrical Stimulation Systems, *Med Eng Phys*, 23:391-399,
   2001.

8. Francisco G, Chae J, Chawla H, Kirshblum S, Zorowitz R,
   Lewis G, Pang S. Electromyogram-triggered neuromuscular
   stimulation for improving the arm function of acute stroke

survivors: a randomised pilot study. *Arch Phys Med Rehabil* 79:5 570-5, 1998.

9. Gentilucci M, Negrotti A, Gangitano M. Planning an action. *Exp Brain Res* 115:116-128, 1997.

10. Glanz M, Klawansky S, Stason W, Berkey C, Chalmers TC. Functional electrostimulation in poststroke rehabilitation: a meta-analysis of the randomised controlled trials. *Arch Phys Med Rehabil* 77:6 549-53, 1996.

11. Hoshimiya N, Naito N, Yajima M, Handa Y. A Multichannel FES System for the Restoration of Motor Functions in High Spinal Cord Injury Patients: A Respiration-Controlled System for Multijoint Upper Extremity. *IEEE Trans Biomed Eng* BME-36:754-760, 1989.

12. Hummelsheim H, Maier-Loth ML, Eickhof C. The functional value of electrical muscle stimulation for the rehabilitation of the hand in stroke patients. *Scand J Rehabil Med* 29:1 3-10, 1997.

13. Ilic M, Vasiljevic D, Popovic DB. A programmable electronic stimulator for FES systems. *IEEE Trans Rehabil Eng* TRE-2:234-239, 1994.

14. Jeannerod M *Intersegmental coordination during reaching at natural visual objects.* In: Long J, Baddeley A (eds.). Lawrence Erlbaum Associates, Hillsdale, NJ, 1981.

15. Jonic S, Jankovic T, Gajic V, Popovic DB. Three machine learning techniques for automatic determination of rules to control locomotion. *IEEE Trans Biomed Eng* BME-46(3):300-310, 1999.

16. Kraft GH, Fitts SS, Hammond MC. Techniques to improve function of the arm and hand in chronic hemiplegia. *Arch Phys Med Rehabil* 73:3 220-7, 1992.

17. Kunkel A, Kopp B, Müller G, Villringer K, Villringer A, Taub E, Flor H. Constraint-induced movement therapy for motor recovery in chronic stroke patients. *Arch Phys Med Rehabil* 80:6 624-8, 1999.

18. Latash ML, Alexander AS, Zatsiorsky VM. The basis of a simple synergy: reconstruction of joint equilibrium trajectories during unrestrained arm movements. *Hum Movt Sci* 18:3-30, 1999..

19. Liberson WF, Holmquest HJ, Scott D, Dow A. Functional electrotherapy: stimulation of the peroneal nerve synchronized with the swing phase of the gait in hemiplegic patients. *Arch Phys Med Rehab* 42:101-105, 1961.

20. Merletti R, Acimovic R, Grobelnik S, Cvilak G. Electrophysiological orthosis for the upper extremity in hemiplegia: feasibility study. *Arch Phys Med Rehabil* 56:12 507-513, 1975.

21. Miltner WH, Bauder H, Sommer M, Dettmers C, Taub E. Effects of constraint-induced movement therapy on patients with chronic motor deficits after stroke: a replication. *Stroke* 30:3 586-92, 1999.

22. Nathan, RH. Control strategies in FNS systems for the upper extremities. *CRC Press Crit Rev Biomed Eng*, 21(6):485-568, 1993.

23. Popovic DB, Popovic MB, Stojanovic A, Pjanovic A, Radosavljevic S, Vulovic D. Clinical Evaluation of the Belgrade grasping system, *Proc 5th Vienna Workshop on FES*, Vienna, 247-250, 1998.

24. Popovic DB, Popovic MB. Belgrade grasping system. *J Electronics* 2:21-28, Banja Luka, 1998.

25. Popovic DB, Sinkjær T. *Control of movement for the physically disabled*, Springer, 2000.

26. Popovic DB, Stojanovic A, Pjanovic A, Radosavljevic S, Popovic MB, Jovic S, Vulovic D. Clinical evaluation of the bionic glove. *Arch Phys Med Rehabil* 80:299-304, 1999.

27. Popovic MB, Jovanovic N, Schwirtlich L. Identification of
5   parameters for control of assistive systems. *J Aut Control*, Belgrade 4:31-45, 1994.

28. Popovic MB, Popovic DB. A new approach to reaching control for tetraplegic subjects. *J Electromyog and Kinesiol* 4:242-253, 1994.

10 29. Popovic MB, Control of upper-extremity neuroprosthesis, *Med Eng Phys*, 2002 (submitted).

30. Popovic MB, Popovic DB, Sinkjær T, Stefanovic A, Schwirtlich L. Restitution of reaching and grasping promoted by functional electrical therapy. *Proc 6th Vienna*
15 *Workshop on FES*, Vienna, September, 210-213, 2001.

31. Popovic MB, Popovic DB. Cloning Biological Synergies Improves Control of Elbow Neuroprosthesis. *IEEE EMB Magazine*, 24(1):74-81, 2001.

32. Popovic, DB, Popovic MB, Sinkjær T. Neurorehabilitation of
20   Upper Extremities in Humans with Sensory-Motor Impairment. *Neuromod*, 5(1):54-67, 2002

33. Potkonjak V, Kostic D, Tzafestas S, Popovic MB, Lazarevic M and Djordjevic G. Human-like behavior of robot arms: general considerations and the handwriting task-Part II:
25   the robot arm in handwriting. *Rob Comp Integr Manuf* 17:317-327, 2001.

34. Prochazka A, Gauthier M, Wieler M, Kenwell Z. The Bionic glove: an electrical stimulator garment that provides controlled grasp and hand opening in quadriplegia. *Arch*
30   *Phys Med Rehabil* 78(6):608-614, 1997.

35. Rebersek S, Vodovnik L. roportionally controlled functional electrical stimulation of hand.. *Arch Phys Med Rehabil* 54:378-382, 1973.

36. Saxena S, Nikolic S, Popovic DB, An EMG-controlled grasping system for tetraplegics, *J Rehabil Res & Develop*, 32:17-24, 1995.

37. Sherrington CS. *The integrative action of the nervous system.* 2nd ed. New Haven CT: Yale University Press, 1947.

38. Smith BT, Peckham PH, Keith MW, Roscoe DD, An externally powered, multichannel, implantable stimulator for versatile control of paralyzed muscle. *IEEE Trans Biomed Eng* BME-34(7):499-508, 1987.

39. Smith BT, Mulcahey BJ, Betz RP. Development of an upper extremity FES system for individuals with C4 tetraplegia. *IEEE Trans Rehab Eng* TRE-4:264-270, 1996.

40. Smith BT, Tang Z, Johnson MW, Pourmehdi S, Gazdik MM, Buckett JR, Peckham PH. An externally powered multichannel, implantable stimulator-telemeter for control of paralyzed muscles. *IEEE Trans Biomed Eng* BME-45:463-475, 1998.

41. Sonde L, Gip C, Fernaeus SE, Nilsson CG, Viitanen M. Stimulation with low frequency (1.7 Hz) transcutaneous electric nerve stimulation (low-tens) increases motor function of the post-stroke paretic arm. *Scand J Rehabil Med* 30:2 95-9, 1998.

42. Sonde L, Kalimo H, Fernaeus SE, Viitanen M. Low TENS treatment on post-stroke paretic arm: a three-year follow-up. *Clin Rehabil* 14:1 14-9, 2000.

43. Sunderland A, Tinson DJ, Bradley EL, Fletcher D, Langton Hewer R, Wade DT. Enhanced physical therapy improves recovery of arm function after stroke. A randomised

controlled trial. *J Neurol Neurosurg Psychiatry* 55:7 530-5, 1992.

44. Taub E, Uswatte G, Pidikiti R. Constraint-Induced Movement Therapy: a new family of techniques with broad application to physical rehabilitation--a clinical review [see comments], *J Rehabil Res Dev* 36:3 237-51, 1999.

45. Tomovic R, Popovic DB, Stein R. *Nonanalytical Methods for Motor Control*, World Sci Publ, Singapore, 1995.

46. Van Kan PLE, Horn KM, Gibson AR. The importance of hand use to discharge of interpositus neurones of the monkey. *J Physiol* (Lond.), 480: 171-190, 1994.

47. Volpe BT, Krebs HI, Hogan N, Edelstein OTR L, Diels C, Aisen M. A novel approach to stroke rehabilitation: robot-elicited sensorimotor stimulation, *Neurology* 54:10 1938-44, 2000.

CLAIMS

1. A method for integrating electrical stimulation and upper extremity exercise in order to improve the physical
5 ability of persons having a disabled upper extremity due to sensory-motor impairment of the central nervous system, said method comprising the steps:

- imposing from the apparatus functional electrical stimulation of neural pathways based on a voluntary command
10 using a stimulation pattern that mimics natural flow of neural activities to the impaired upper extremity,

- generating the missing components of a functional movement in parallel with the voluntary exercising of the same functional movement based on the said patterned
15 stimulation of the efferent neural pathways time-synchronized with volitional movement,

- enhancing the afferent input by the said patterned electrical stimulation in time synchrony with the biological afferent activity caused by the functional movement of the
20 limb.

2. A method according to claim 1, where the electrical stimulation is provided from the stimulator at a number of the bodily locations by means of surface electrodes.

25

3. A method according to claim 1 or claim 2, where the efferent pathways are pathways from the spinal cord of the disabled person to a muscle in the arm or hand of the disabled person.

30

4. A method according to claim 1, where a control algorithm is incorporated into the controller, said control algorithm mimicking the natural sequence of activation of muscles responsible for functional movements; mimicking
5 relating to triphasic activity of agonists and antagonists and controlling the level of co-contraction of agonists and antagonists.

5. A method according to any of preceding claims of
10 using a voluntary movement in the same upper limb as a source to drive in an open-loop control scheme the activation of more distal parts of the arm.

6. A method according to any of preceding claims, where
15 the afferent pathways are pathways from the sensory system of the body of the disabled person to the spinal cord of the person.

7. A method according to claim 1 where the steps are
20 repeated so that the electrical stimulation is for a prolonged time providing a strong afferent input that is correlated with the propriceptive and exteroceptive inputs caused by the voluntary movement and contacts with the environment.

25

8. Apparatus for use in the integrated electrical stimulation and upper extremity exercise in order to improve the physical ability of the upper limb of a disabled person, said apparatus comprising a stimulator for providing
30 electrical signal outputs via a number of stimulation channels, and a number of electrodes for placement in physical contact with the body of the disabled person and

means for connecting said electrodes to said stimulator, and a controller providing instructions to said stimulator and implementing a control algorithm that causes the stimulator to provide via said channels stimulation patterns of said

5 electrical signals which induce muscle movements in use which mimic the timing and modulation of muscles typically active in able-bodied humans that are available for surface activation with electrical stimulation in persons with impairment, said signals including non-simultaneous peaks of

10 activation of agonist and antagonist muscles during a single direction of movement (triphasic pattern) and appropriate coactivation of agonist and antagonist muscles needed for a desired functional movement.

15   9.   Apparatus according to claim 8, for producing manipulation and grasping of objects with an impaired hand.

         10.   Apparatus according to claim 8 or claim 9, where the controller communicates with a number of stimulators,

20 said stimulators comprising lead communication, alternatively or supplementary wireless communication channels between the controller and stimulation points.

         11.   An apparatus according to any of claims 8 to 10,

25 where the apparatus is intended for stimulating and controlling fingers, thumb, and forearm of the disabled person, and where the number of stimulator channels comprises at least one channel for the finger flexors, at least one channel for the finger extensors, at least one

30 channel for thumb extension/adduction, and at least one channel for thumb opposition/flexion.

12. Apparatus as claimed in any one of claims 8 to 11, further comprising a shoulder angle sensor for determining the angle or rate of change of the angle between the upper arm and a reference line, wherein said controller is adapted

5 to initiate and to regulate a said control algorithm inducing a sequence of reaching, grasping, moving, holding, returning and releasing an object in response to measurement or calculation of said rate of change based upon the output of said shoulder sensor.

10

13. Use of the apparatus according to any of claims 8-10 for improving the physical ability of persons having disabled limbs due to sensory-motor impairment in the brain of the person caused by a lesion of the central nervous

15 system of the person, where the improvement relates to long-term changes of ability to perform movement without the stimulation after the treatment.

14. Use of apparatus for temporary therapeutic

20 applications in persons with sensory motor deficit of an upper limb within the intensive physical exercise, said therapeutic application augmenting and/or generating the missing movement of the hand/arm.
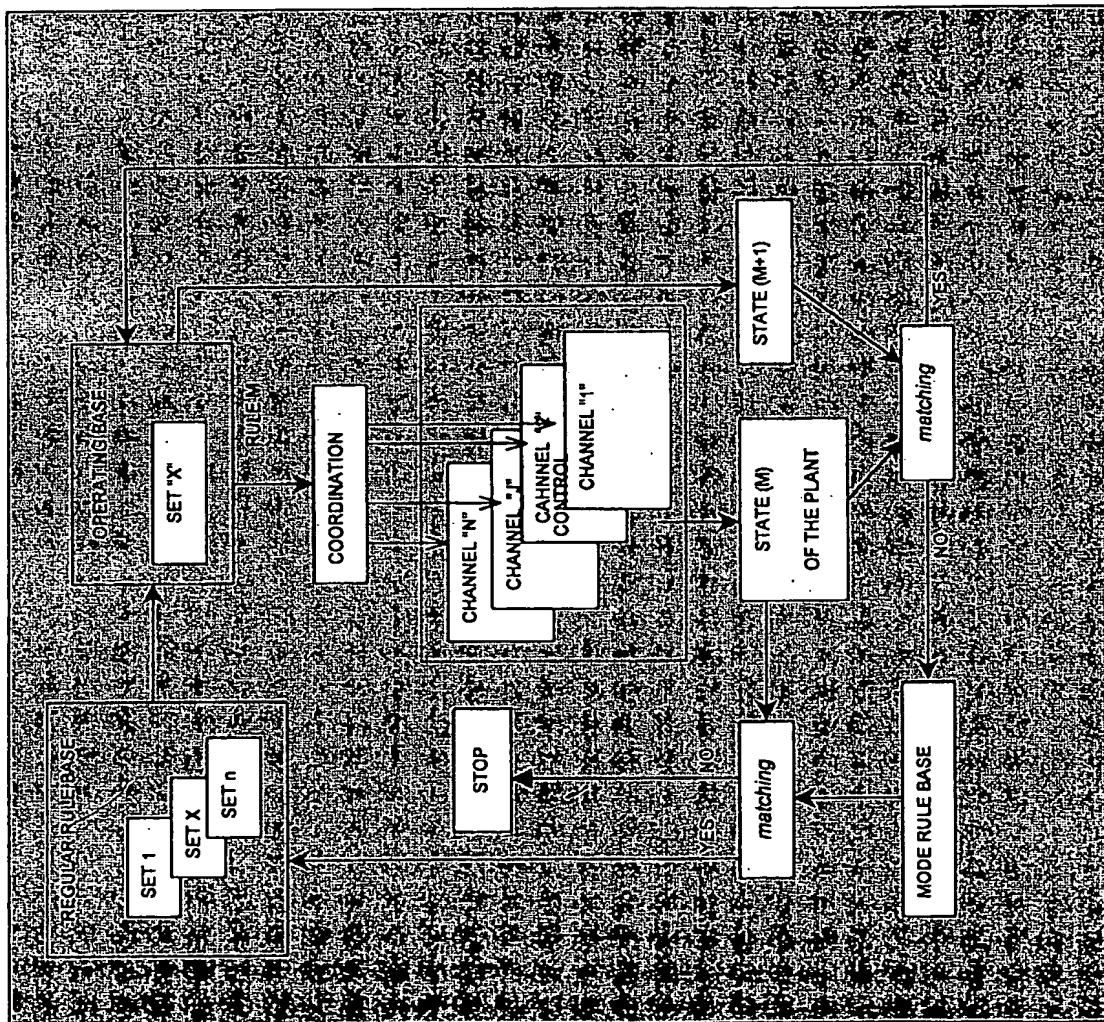
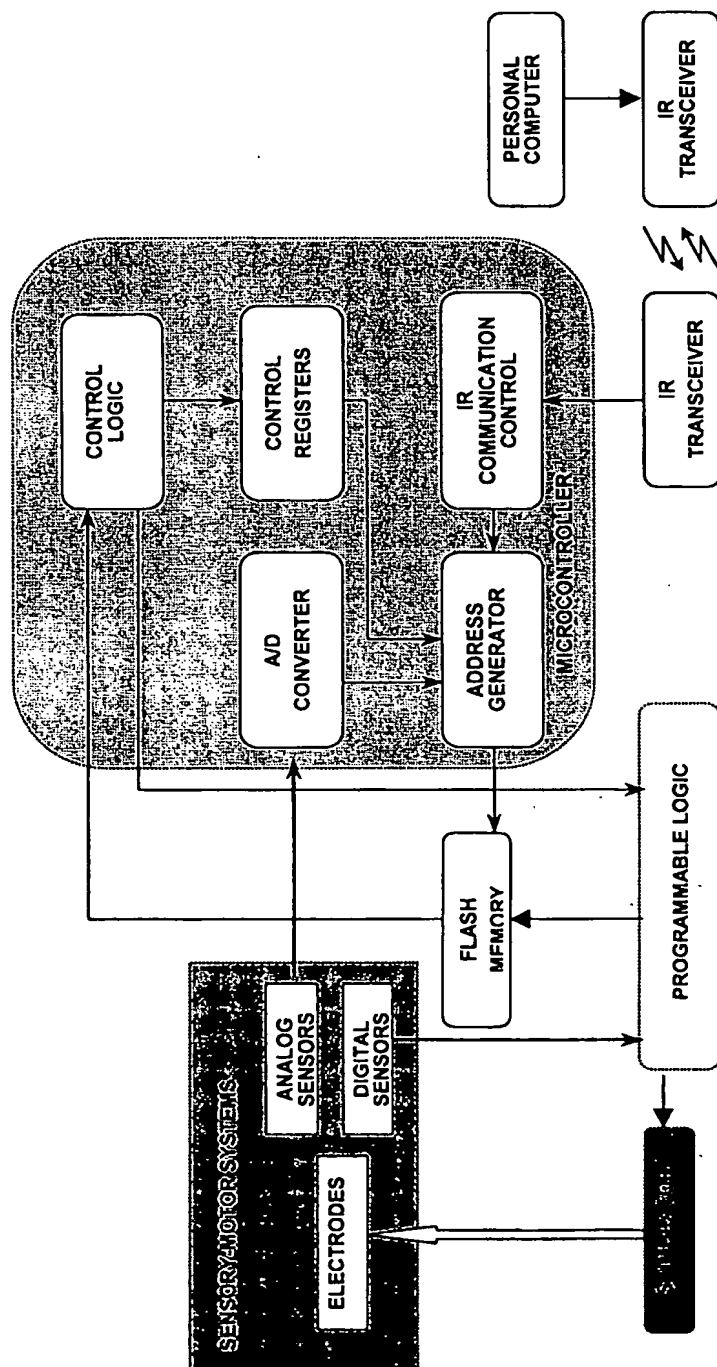Fig. 1: Organization of the rule-based synergistic control at coordination and actuation levels for FETS

Fig. 2: Schema of the central stimulator/controller for Functional Electrical Therapy System (FETS)
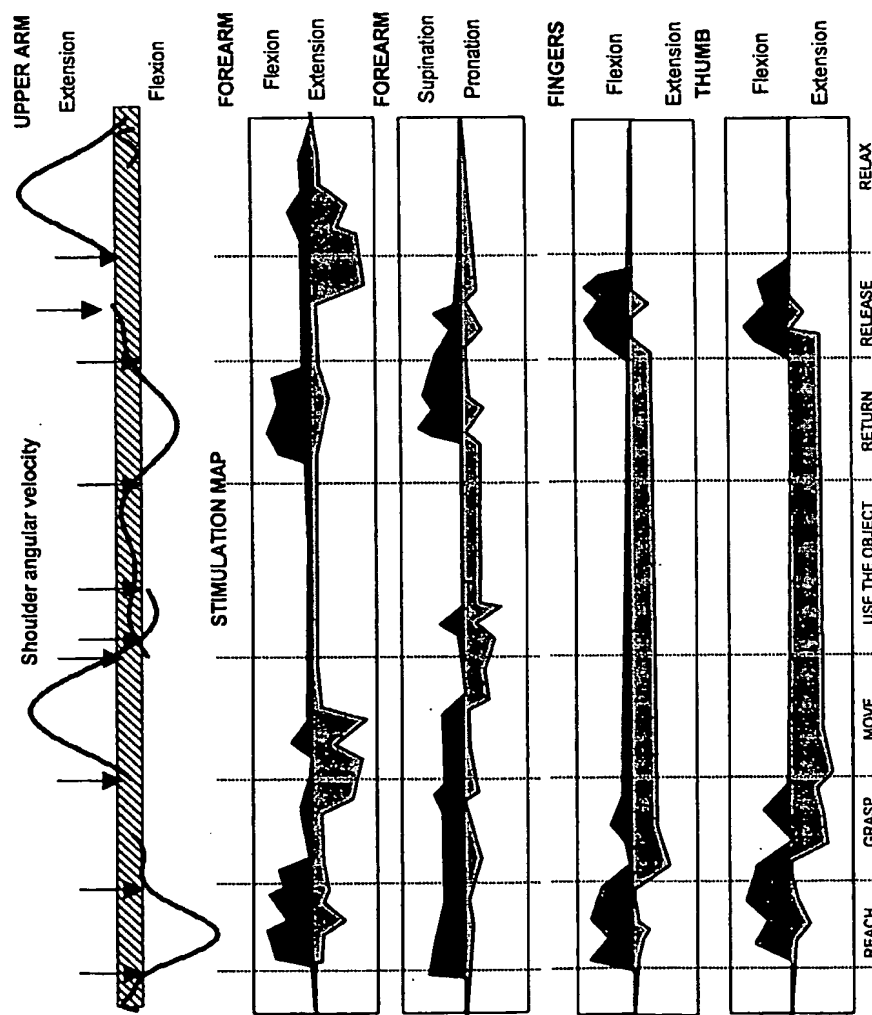
Fig. 3: Stimulation map for drinking from a full juice-can. Dark areas relate to extension, adduction and pronation, light areas relate to flexion, abduction and supination. Activations are normalized to the maximum. Spatial synergy was used for forearm flexion/extension, and temporal synchrony for all four joint rotations.
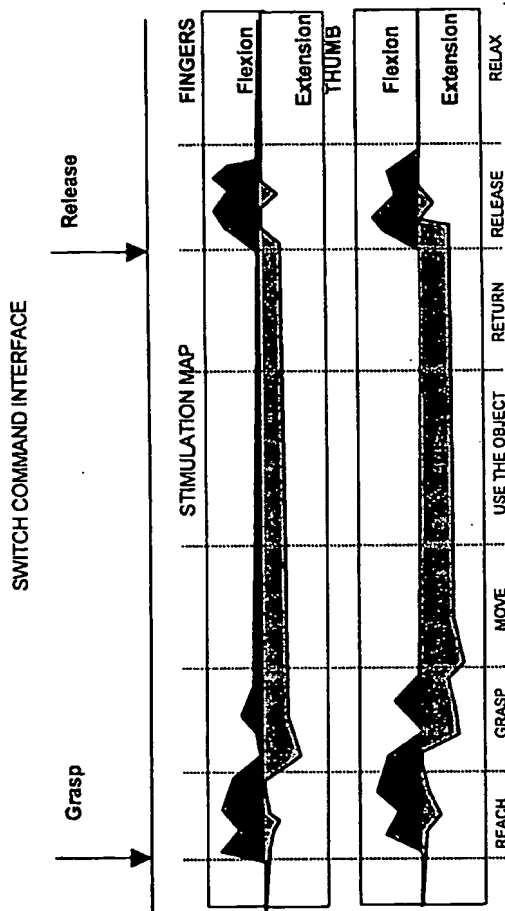
Fig. 4: Stimulation map for drinking from a full juice-can. Dark areas relate to extension and light areas relate to flexion. Activations are normalized to the maximum level. Temporal synchrony was applied for all of the grasp and release functions. It is anticipated that the subject is able to control his/her shoulder and elbow joints, and perform necessary trunk and head position adjustments.

INTERNATIONAL SEARCH REPORT

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7   A61N1/36

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7   A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 580 569 A (PETROFSKY JERROLD S) 8 April 1986 (1986-04-08) the whole document	8-12
X	US 5 330 516 A (NATHAN ROGER H) 19 July 1994 (1994-07-19) cited in the application the whole document	8,9
X	US 5 167 229 A (PECKHAM PAUL H ET AL) 1 December 1992 (1992-12-01) cited in the application the whole document	8-12
X	US 4 976 264 A (PETROFSKY STEVEN H) 11 December 1990 (1990-12-11) the whole document	8

-/--

| X | Further documents are listed in the continuation of box C. | | X | Patent family members are listed in annex. |

° Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
22 August 2002	28/08/2002

Name and mailing address of the ISA	Authorized officer
European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Ferrigno, A

Form PCT/ISA/210 (second sheet) (July 1992)

Category *	Citation of document, with indication,where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 556 214 A (PETROFSKY JERROLD S ET AL) 3 December 1985 (1985-12-03) the whole document	8
A	US 4 642 769 A (PETROFSKY JERROLD S) 10 February 1987 (1987-02-10) the whole document	8

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

INTERNATIONAL SEARCH REPORT

Box I	Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. [X] Claims Nos.:   1-7,13,14
because they relate to subject matter not required to be searched by this Authority, namely:

> Rule 39.1(iv) PCT - Method for treatment of the human or animal body by therapy

2. [ ] Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:

3. [ ] Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II	Observations where unity of Invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple Inventions In this International application, as follows:

1. [ ] As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. [ ] As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. [ ] As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. [ ] No required additional search fees were timely paid by the applicant. Consequently, this International Search Report Is restricted to the invention first mentioned in the claims; it Is covered by claims Nos.:

Remark on Protest

[ ] The additional search fees were accompanied by the applicant's protest.

[ ] No protest accompanied the payment of additional search fees.

Form PCT/ISA/210 (continuation of first sheet (1)) (July 1998)

Patent document cited in search report		Publication date	Patent family member(s)		Publication date
US 4580569	A	08-04-1986	CA	1264814 A1	23-01-1990
			EP	0145503 A2	19-06-1985
			JP	60153875 A	13-08-1985
US 5330516	A	19-07-1994	IL	97701 A	29-06-1995
			AT	156690 T	15-08-1997
			AU	651675 B2	28-07-1994
			AU	1384992 A	01-10-1992
			CA	2064151 A1	29-09-1992
			DE	69221521 D1	18-09-1997
			DE	69221521 T2	12-02-1998
			DK	506398 T3	09-03-1998
			EP	0506398 A1	30-09-1992
			ES	2106135 T3	01-11-1997
			HU	214425 B	30-03-1998
			IE	920942 A1	07-10-1992
			JP	3251632 B2	28-01-2002
			JP	5076555 A	30-03-1993
			ZA	9202233 A	25-11-1992
US 5167229	A	01-12-1992	US	6026328 A	15-02-2000
US 4976264	A	11-12-1990	WO	9118643 A1	12-12-1991
			WO	9116105 A1	31-10-1991
			US	4996987 A	05-03-1991
US 4556214	A	03-12-1985	US	4480830 A	06-11-1984
			CA	1209001 A1	05-08-1986
			EP	0103490 A2	21-03-1984
			JP	1712654 C	27-11-1992
			JP	3076951 B	09-12-1991
			JP	59146669 A	22-08-1984
US 4642769	A	10-02-1987	NONE		